

# EXspect 271 NIR backscattering sensor in compact design





- » Compact design with integrated amplifier and touch display
- » %-turbidity or customer defined unit
- » Durable sapphire lens
- » Hygienic Design, CIP/SIP-capable
- » LED light source guarantees a durable and stable signal
- » Easy parameterization via display or software EXpert

EXspect 271 is a high precisely compact NIR turbidity sensor monitoring production processes in the food industry, e.g. in dairies, as well as in many ranges of process and chemical applications and waste water.


## Specifications

Measuring range max.	0-100 %
Resolution	0,1 %
Accuracy	± 1,5 % from measurement value
Reproducibility	≤ 1 % from final value
Wavelength	850 nm
Light source	LED
Material	Stainless steel 1.4435 (316L)
Surface	e-polished Ra <0,37 µm
Lens	Sapphire
Supply voltage	24 V DC
Contact	NO or NC configurable 150 mA
Input contact	zeroing
Process connection	Thread G1/2"
Process temperature	-10... 90 °C, 141 °C max. 2 hours (SIP cycle)
Process pressure	-1... 20 bar
Electrical connection	M12 connector 5-pin or 8-pin (digital parameterizable)
Cable length	2 m / 5 m
Interfaces	4 ... 20 mA with add. switching contact
Parameterization	Software EXpert
Protection class	IP69

## Typical Measurements

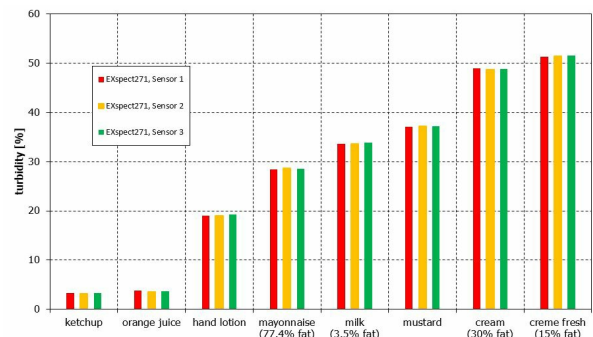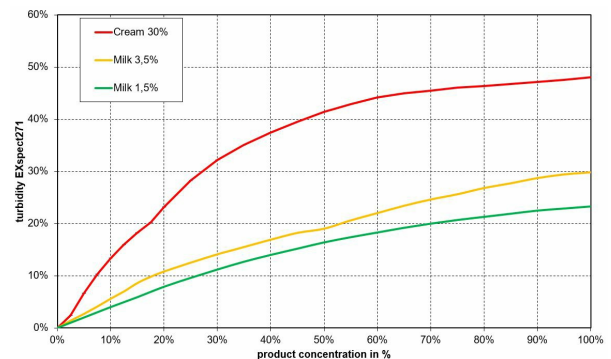

## EXspect 271 NIR backscattering sensor in compact design

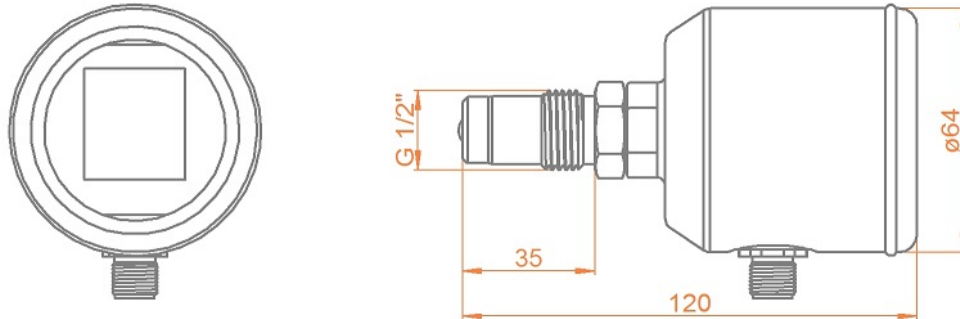

### Ordercode

Code	Measuring range	Delivery
A	0...100% turbidity	3 weeks

Code	Material (wetted parts)	Delivery
4435	Stainless steel 1.4435 / 316L	3 weeks

Code	Sealing material (wetted sealings)	Delivery
MET	Metal sealing (without elastomer)	3 weeks

Code	Process connection	Delivery
G12	Thread G1/2"	3 weeks

Code	Interface	Delivery
AS	Analogue 4...20 mA / M12 5 pin	3 weeks
AD	Analogue 4...20 mA / digitally parameterizable / M12 8 pin	3 weeks

Code	Display	Delivery
1	With integrated display	3 weeks

### Accessories



Weld-in socket and process adapter



EXcap 120 - Set of reference normals for in-field verification of measurements and calibration